


Cerner Flash

Coming 8/11/2022

Acute Nursing-New Rule for External Catheters

As we note an increase in external catheter utilization, we have created a task in Cerner to help remind staff when the external urinary catheter needs to be changed. Utilizing the task will lead the nurse to the proper band in iView to complete the documentation of the catheter change. The task will affect adult patients with a Inpatient, Observation or Outpatient in a bed status.

1. Open iView and navigate to Adult Lines-Devices>choose Urine External/Suprapubic/Intermittent>create dynamic group>choose Urine device type-External>Urine Device type (choices will default depending on the documented sex of the patient-choose the appropriate option and click OK.

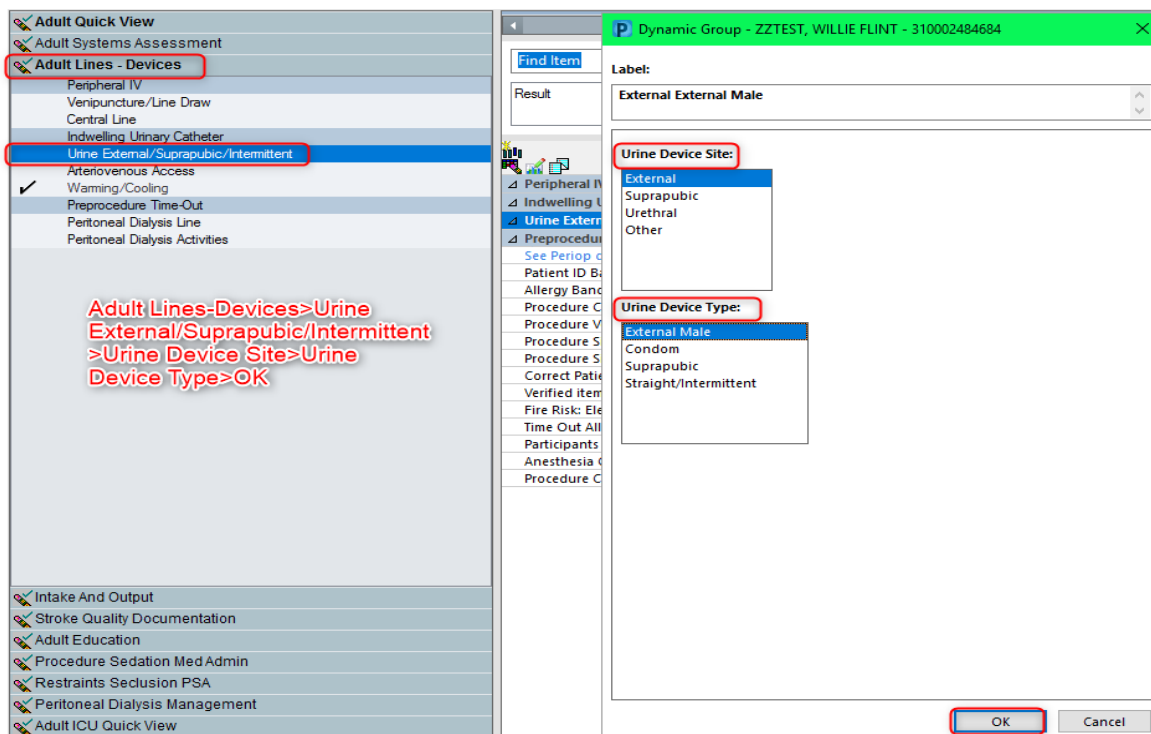

2. An order will be created based off the creation of the dynamic group. The frequency of the order to change the catheter will vary depending on the documented sex of the patient. Male-q24h and Female is q12h

Patient Care			
<input checked="" type="checkbox"/>	External Urine Device Change - Male	Ordered	07/25/22 10:33:27 EDT, Q24H Please change external urine device.

Order is automatically created with frequency for changing the catheter based on the sex of the patient. The nurse will be tasked based on the frequency of the order.

Cerner Flash

3. Task will display appropriately based on the frequency of the order.

External Urine Device Change - Male External Catheter Care - Male 08/03/22 11:00:00 EDT
 Comment: Please change external urine device.

4. Utilizing the task to document will direct you to proper documentation fields to ensure you complete all appropriate documentation.

Activity View

Urine External/Suprapubic/Intermittent

Urine External/Suprapubic/Intermittent

The task will take you directly to the documentation fields to complete the appropriate documentation

Find Item Critical High Low Abnormal

Result	Comments	Flag	Date																																												
8/3/2022 12:42 EDT																																															
<div style="border: 2px solid red; padding: 5px;"> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td colspan="2">Urine External/Suprapubic/Intermittent</td> <td style="text-align: center;"><input checked="" type="checkbox"/></td> <td></td> </tr> <tr> <td colspan="2">Urine External/Suprapubic/Intermittent</td> <td style="text-align: center;"><input checked="" type="checkbox"/></td> <td></td> </tr> <tr> <td colspan="2">External External Male</td> <td style="text-align: center;"><input checked="" type="checkbox"/></td> <td></td> </tr> <tr> <td>Urine Device Activity:</td> <td>Urine Device Activity:</td> <td></td> <td style="text-align: right;">✕</td> </tr> <tr> <td>Urine Device Drainage System:</td> <td>Assessment</td> <td></td> <td></td> </tr> <tr> <td>Urine Device Management:</td> <td>Changed</td> <td></td> <td></td> </tr> <tr> <td>Urine Device Patient Response:</td> <td>Discontinued</td> <td></td> <td></td> </tr> <tr> <td>Urine Device Unexpected Events:</td> <td>Placed</td> <td></td> <td></td> </tr> <tr> <td>Urine Device Site Condition:</td> <td>Present on admission</td> <td></td> <td></td> </tr> <tr> <td>Urine Device Irrigant In:</td> <td> mL Straight/Intermittent</td> <td></td> <td></td> </tr> <tr> <td>Urine Device Output:</td> <td> mL Other</td> <td></td> <td></td> </tr> </table> </div>				Urine External/Suprapubic/Intermittent		<input checked="" type="checkbox"/>		Urine External/Suprapubic/Intermittent		<input checked="" type="checkbox"/>		External External Male		<input checked="" type="checkbox"/>		Urine Device Activity:	Urine Device Activity:		✕	Urine Device Drainage System:	Assessment			Urine Device Management:	Changed			Urine Device Patient Response:	Discontinued			Urine Device Unexpected Events:	Placed			Urine Device Site Condition:	Present on admission			Urine Device Irrigant In:	mL Straight/Intermittent			Urine Device Output:	mL Other		
Urine External/Suprapubic/Intermittent		<input checked="" type="checkbox"/>																																													
Urine External/Suprapubic/Intermittent		<input checked="" type="checkbox"/>																																													
External External Male		<input checked="" type="checkbox"/>																																													
Urine Device Activity:	Urine Device Activity:		✕																																												
Urine Device Drainage System:	Assessment																																														
Urine Device Management:	Changed																																														
Urine Device Patient Response:	Discontinued																																														
Urine Device Unexpected Events:	Placed																																														
Urine Device Site Condition:	Present on admission																																														
Urine Device Irrigant In:	mL Straight/Intermittent																																														
Urine Device Output:	mL Other																																														