


Cerner Flash

Date 9/14/23

<<New Definity Kit Contrast Charge>> <<Contrast Charges – Non-Invasive PowerForm >>

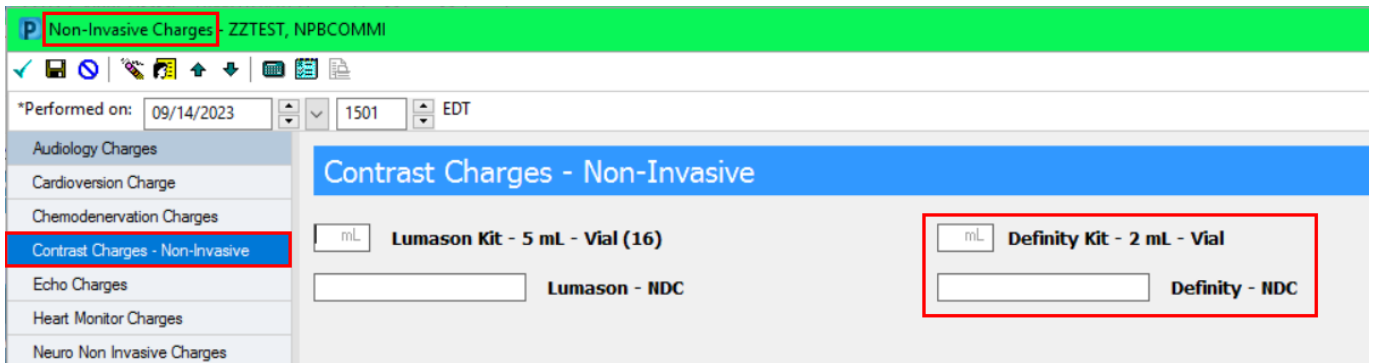

The screenshot shows a Cerner PowerForm titled "Non-Invasive Charges - ZZTEST, NPBCOMMI". The form includes a date field for "Performed on:" set to 09/14/2023 and a time field set to 1501 EDT. A left-hand menu lists various charge categories, with "Contrast Charges - Non-Invasive" selected. The main content area is titled "Contrast Charges - Non-Invasive" and contains two columns of input fields. The left column has a "mL" input field, a text label "Lumason Kit - 5 mL - Vial (16)", and a text label "Lumason - NDC" with an empty input field below it. The right column has a "mL" input field, a text label "Definity Kit - 2 mL - Vial", and a text label "Definity - NDC" with an empty input field below it. Red boxes highlight the "Non-Invasive Charges" menu item and the "mL" input fields in both columns.

NDC needed format: XXXXX-XXXX-XX

If a manufacturer's NDC is not in that format, the leading zeros need to be added to the appropriate section. For Cerner, you do not report the dashes when manually entering the documentation.

For example:

1542-130-01

01542-0130-01

Manually entered as 01542013001